



**APPLICATION FOR REGISTRATION AS A REGISTERED SERVICE COMPANY**

Public Service Commission  
SFN 51277 (2/2014)



**TYPE OR PRINT - AN INCOMPLETE OR ILLEGIBLE APPLICATION WILL BE REJECTED**

Name of Company <b>Hobbs Inc.</b>	Email Address <b>hobbsone@btinet.net</b>	Application Date <b>5/2/14</b>	
Mailing Address <b>2389 Business Loop I-94</b>	City <b>Mandan</b>	State <b>ND</b>	Zip Code <b>58554</b>
Telephone Number <b>701-663-6363</b>	Cell Phone Number	Fax Number <b>701-663-9220</b>	

**Select below all device types your company will certify:**

Scales (include maximum capacity, if applicable)	Liquid (include maximum flow rate, if applicable)
<input type="checkbox"/> 1. Rail <input type="checkbox"/> 2. Truck <input type="checkbox"/> 3. Livestock <input type="checkbox"/> 4. Hopper: Max. Capacity: _____ <input type="checkbox"/> 5. Belt <input type="checkbox"/> 6. Over 30 lbs.: Max. Capacity: _____ <input type="checkbox"/> 7. 30 lbs. or less <input type="checkbox"/> 8. Class II (indicate on your calibration report which weight kit is Class II certified) <input type="checkbox"/> 9. Other: Please List:	<input checked="" type="checkbox"/> 1. Retail Fuel (less than 20 gal. per minute) <input checked="" type="checkbox"/> 2. High Flow Retail Fuel (20 gal. per minute or greater) <input checked="" type="checkbox"/> 3. Vehicle Tank: Max. Flow Rate: <u>100</u> <input checked="" type="checkbox"/> 4. Stationary Bulk (fuel or oil): Max. Flow Rate: <u>100</u> <input type="checkbox"/> 5. LPG <input type="checkbox"/> 6. Stationary LPG <input type="checkbox"/> 7. Fertilizer: Max. Flow Rate: _____ <input type="checkbox"/> 8. Chemical <input type="checkbox"/> 9. Anhydrous <input type="checkbox"/> 10. Loading Rack <input type="checkbox"/> 11. Other: Please List:

**List below all persons employed by your company as a North Dakota Registered Service Person and the device types they are registered to certify (attach a separate sheet to list additional employees):**

Permit No.	Employee	Device Types Registered to Certify (list using device type numbers from above)
e.g. 1001	e.g. John Doe	e.g. Scales - 2, 3, 6, 8; e.g. Liquid - 1, 2, 6
<b>1340</b>	<b>James Munns</b>	<b>1, 2, 3, 4</b>



List below all field standards (attach current calibration reports):

100 gal Liquid Prover	
5gal SS Seraphin	
5gal SS Seraphin	
5gal Seraphin mild steel	
5gal Seraphin mild steel	


Additional Application Items (initial where appropriate):

Standardized Test Report	<input checked="" type="checkbox"/> Copy enclosed <input type="checkbox"/> No change in report filed previously
Tested and Approved Sticker	<input type="checkbox"/> Copy enclosed <input checked="" type="checkbox"/> No change in sticker filed previously
Photocopy of Crimped Lead Wire Seal	<input type="checkbox"/> Copy enclosed <input type="checkbox"/> No change in crimped lead wire seal filed previously

Public Company Listing:

Include my company information on your registered service company list for public contact.  
 Yes     No

I am TODD KRENELKA, and have authority to represent this company. By signing this application, I declare that I have examined this form and accompanying documentation, and to the best of my knowledge and belief, the facts stated and documentation provided is true, correct, and complete.

  
Signature

Send Completed Application and Related Documents To:

Public Service Commission  
600 E Boulevard Ave Dept 408  
Bismarck ND 58505-0480  
Telephone: (701) 328-2400  
Fax: (701) 328-2410



Receipt Date: April 25, 2014  
Test Date: April 25, 2014  
Report Date: April 25, 2014

State Test No.: 332456  
Serial No.: 35213-8  
Bar Code: 201130

## Calibration Report

HOBBS, INC.  
2389 BUSINESS LOOP I-94  
MANDAN, ND 58554  
Contact: JEFF ENGEL  
Phone: 701-663-6363  
PO Number: None  
SOP: 32  
Technician ID: 08

Item(s) Submitted: 5 Gallon Measure  
Manufacturer: Seraphin  
Material: ss  
Equipment Number: None  
Condition: Good  
Temperature: 19.2°C  
Pressure: 731.4 mmHg  
Relative Humidity: 49. %

Nominal Volume		Error (in <sup>3</sup> )	Volume	Uncertainty (in <sup>3</sup> )	Coefficient of Expansion(1/°F)
			Contained At Zero Line (gallons)		
5 gal	As Found	0.05	5.0002	0.62	0.0000265
	As Left	0.05	5.0002	0.62	

Neck Calibration: No neck calibration was done at this time.


This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of flow and at a reference temperature of 60°F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.

Results apply to item identified in this report only.


Nils Fleming

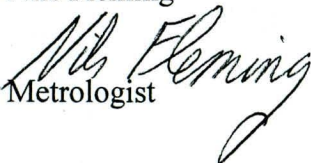

Metrologist

Reviewed by:

Mark Nicollet



Approved Signatory



Weights & Measures Metrology Laboratory  
 14305 Southcross Drive #150  
 Burnsville, MN 55306-7008  
 651.539.1555 FAX 651.539.1553



Receipt Date: April 25, 2014  
 Test Date: April 25, 2014  
 Report Date: April 25, 2014

State Test No.: 332457  
 Serial No.: 38086  
 Bar Code: 201128

## Calibration Report

HOBBS, INC.  
 2389 BUSINESS LOOP I-94  
 MANDAN, ND 58554  
 Contact: JEFF ENGEL  
 Phone: 701-663-6363  
 PO Number: None  
 SOP: 32  
 Technician ID: 08

Item(s) Submitted: 5 Gallon Measure  
 Manufacturer: Seraphin  
 Material: ss  
 Equipment Number: None  
 Condition: Good  
 Temperature: 19.2°C  
 Pressure: 731.4 mmHg  
 Relative Humidity: 49. %

Nominal Volume		Error (in <sup>3</sup> )	Volume Contained		Coefficient of Expansion(°F)
			At Zero Line (gallons)	Uncertainty (in <sup>3</sup> )	
5 gal	As Found	-0.05	4.9998	0.62	0.0000265
	As Left	-0.05	4.9998	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of flow and at a reference temperature of 60°F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.

Results apply to item identified in this report only.

Nils Fleming  
  
 Metrologist

Reviewed by:  
 Mark Nicollet  
  
 Approved Signatory





Receipt Date: April 25, 2014  
Test Date: April 25, 2014  
Report Date: April 25, 2014

State Test No.: 332458  
Serial No.: 40713  
Bar Code: 201131

## Calibration Report

HOBBS, INC.  
2389 BUSINESS LOOP I-94  
MANDAN, ND 58554  
Contact: JEFF ENGEL  
Phone: 701-663-6363  
PO Number: None  
SOP: 32  
Technician ID: 08

Item(s) Submitted: 5 Gallon Measure  
Manufacturer: Seraphin  
Material: ms  
Equipment Number: None  
Condition: Good  
Temperature: 19.2°C  
Pressure: 731.4 mmHg  
Relative Humidity: 49. %

Nominal Volume		Error (in <sup>3</sup> )	Volume Contained		Coefficient of Expansion(°F)
			At Zero Line (gallons)	Uncertainty (in <sup>3</sup> )	
5 gal	As Found	-0.27	4.9988	0.62	0.0000186
	As Left	-0.27	4.9988	0.62	

Neck Calibration: No neck calibration was done at this time.


This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of flow and at a reference temperature of 60°F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.

Results apply to item identified in this report only.

Nils Fleming

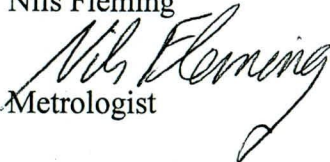

Metrologist

Reviewed by:

Mark Nicollet



Approved Signatory



Weights & Measures Metrology Laboratory  
 14305 Southcross Drive #150  
 Burnsville, MN 55306-7008  
 651.539.1555 FAX 651.539.1553



Receipt Date: April 25, 2014  
 Test Date: April 25, 2014  
 Report Date: April 25, 2014

State Test No.: 332459  
 Serial No.: 45206  
 Bar Code: 201129

## Calibration Report

HOBBS, INC.  
 2389 BUSINESS LOOP I-94  
 MANDAN, ND 58554  
 Contact: JEFF ENGEL  
 Phone: 701-663-6363  
 PO Number: None  
 SOP: 32  
 Technician ID: 08

Item(s) Submitted: 5 Gallon Measure  
 Manufacturer: Seraphin  
 Material: ms  
 Equipment Number: None  
 Condition: Good  
 Temperature: 19.2°C  
 Pressure: 731.4 mmHg  
 Relative Humidity: 49. %

Nominal Volume		Error (in <sup>3</sup> )	Volume Contained		Coefficient of Expansion(/°F)
			At Zero Line (gallons)	Uncertainty (in <sup>3</sup> )	
5 gal	As Found	0.66	5.0028	0.62	0.0000186
	As Left	-0.15	4.9994	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of flow and at a reference temperature of 60°F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.

Results apply to item identified in this report only.

Nils Fleming  
  
 Metrologist

Reviewed by:  
 Mark Nicolle  
  
 Approved Signatory



Weights & Measures Metrology Laboratory  
 14305 Southcross Drive #150  
 Burnsville, MN 55306-7008  
 651.539.1555 FAX 651.539.1553

Receipt Date: April 25, 2014  
 Test Date: April 25, 2014  
 Report Date: April 25, 2014

State Test No.: 332455  
 Serial No.: 1362  
 Bar Code: 201127

## Calibration Report

HOBBS, INC.  
 2389 BUSINESS LOOP I-94  
 MANDAN, ND 58554  
 Contact: JEFF ENGEL  
 Phone: 701-663-6363  
 PO Number: None  
 SOP: 33  
 Technician ID: 08

Item(s) Submitted: 100 Gallon Prover  
 Manufacturer: Gas Service & Supply  
 Material: ss  
 Description: Dry Bottom  
 Condition: Good  
 Temperature: 19.7°C  
 Pressure: 731.1 mmHg  
 Relative Humidity: 44. %

Nominal Volume		Volume (gallons)	Error (in <sup>3</sup> )	Uncertainty (in <sup>3</sup> )	Coefficient of Expansion(/°F)
100 gal	As Found	99.991	-2.2	3.0	0.0000265
	As Left	99.991	-2.2	3.0	

Neck Calibration: No neck calibration was done at this time.

This prover has been calibrated as a "to contain after wet down" vessel with a drain time of 30 seconds after cessation of flow and at a reference temperature of 60°F.

The prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.

Results apply to item identified in this report only.

Nils Fleming


Metrologist

Reviewed by:  
 Mark Nicollet

Approved Signatory





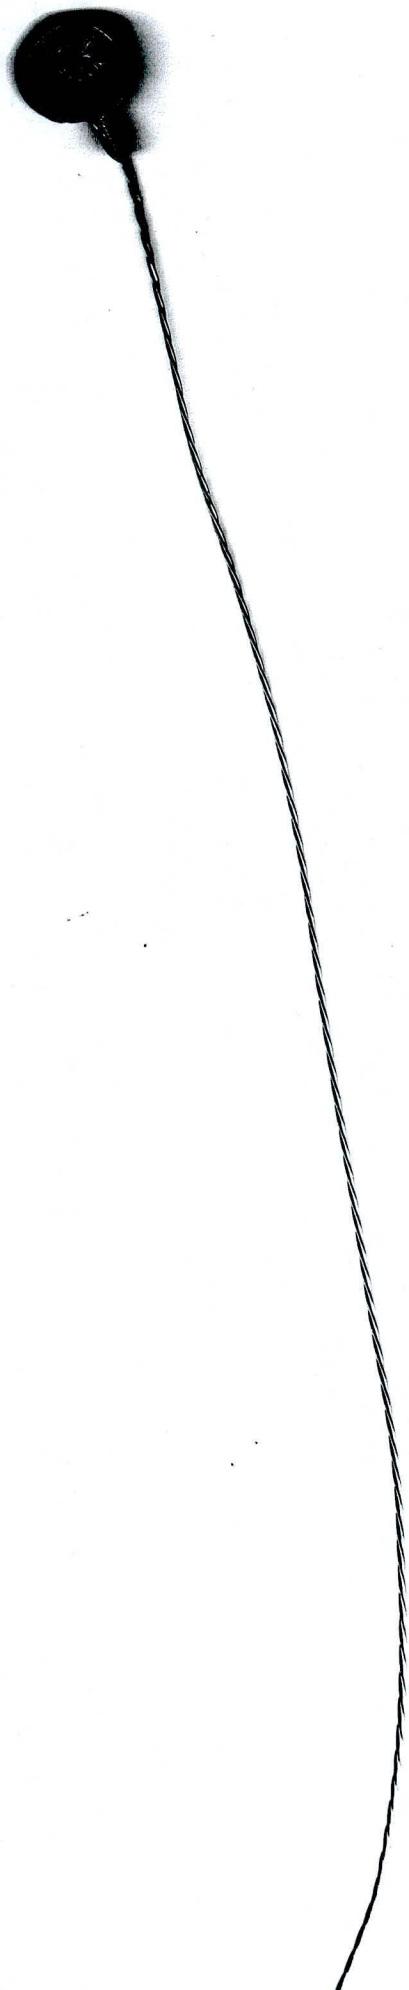

RECEIVED  
MAY 19 2014  
ND Public  
Service  
Commission