



APPLICATION FOR REGISTRATION AS A REGISTERED SERVICE COMPANY

Public Service Commission
SFN 51277 (2/2014)



TYPE OR PRINT - AN INCOMPLETE OR ILLEGIBLE APPLICATION WILL BE REJECTED

Name of Company Petroleum Calibration Service	Email Address PetroleumCalibration@gmail.com	Application Date 7/30/14	
Mailing Address 203 East Hwy 61	City Estok	State ND	Zip Code 55733
Telephone Number 218 213 6556	Cell Phone Number 218 213 6556	Fax Number	

Select below all device types your company will certify:

Scales (include maximum capacity, if applicable)	Liquid (include maximum flow rate, if applicable)
<input type="checkbox"/> 1. Rail <input type="checkbox"/> 2. Truck <input type="checkbox"/> 3. Livestock <input type="checkbox"/> 4. Hopper: Max. Capacity: _____ <input type="checkbox"/> 5. Belt <input type="checkbox"/> 6. Over 30 lbs.: Max. Capacity: _____ <input type="checkbox"/> 7. 30 lbs. or less <input type="checkbox"/> 8. Class II (indicate on your calibration report which weight kit is Class II certified) <input type="checkbox"/> 9. Other: Please List:	<input checked="" type="checkbox"/> 1. Retail Fuel (less than 20 gal. per minute) <input checked="" type="checkbox"/> 2. High Flow Retail Fuel (20 gal. per minute or greater) <input type="checkbox"/> 3. Vehicle Tank: Max. Flow Rate: _____ <input type="checkbox"/> 4. Stationary Bulk (fuel or oil): Max. Flow Rate: _____ <input type="checkbox"/> 5. LPG <input type="checkbox"/> 6. Stationary LPG <input type="checkbox"/> 7. Fertilizer: Max. Flow Rate: _____ <input type="checkbox"/> 8. Chemical <input type="checkbox"/> 9. Anhydrous <input type="checkbox"/> 10. Loading Rack <input type="checkbox"/> 11. Other: Please List:

List below all persons employed by your company as a North Dakota Registered Service Person and the device types they are registered to certify (attach a separate sheet to list additional employees):

Permit No.	Employee	Device Types Registered to Certify (list using device type numbers from above)
e.g. 1001	e.g. John Doe	e.g. Scales - 2, 3, 6, 8; e.g. Liquid - 1, 2, 6
1625	Eyona Lewis	Liquid 1 2

Continued on Page 2

List below all field standards (attach current calibration reports):

Scaphin 5 Gal Provers	
S/N 49433A 49433-B 49433-C	
00-13657-15	




Additional Application Items (initial where appropriate):

Standardized Test Report	<input type="checkbox"/> Copy enclosed <input checked="" type="checkbox"/> No change in report filed previously
Tested and Approved Sticker	<input type="checkbox"/> Copy enclosed <input checked="" type="checkbox"/> No change in sticker filed previously
Photocopy of Crimped Lead Wire Seal	<input type="checkbox"/> Copy enclosed <input checked="" type="checkbox"/> No change in crimped lead wire seal filed previously

Public Company Listing:


Include my company information on your registered service company list for public contact.
 Yes No

I am Eugene Lewis, and have authority to represent this company.
By signing this application, I declare that I have examined this form and accompanying documentation, and to the best of my knowledge and belief, the facts stated and documentation provided is true, correct, and complete.


Signature

Send Completed Application and Related Documents To:

Public Service Commission
600 E Boulevard Ave Dept 408
Bismarck ND 58505-0480
Telephone: (701) 328-2400
Fax: (701) 328-2410

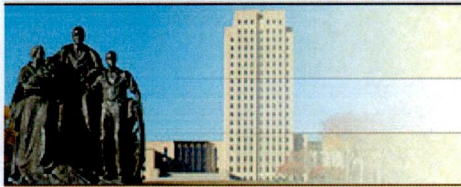

SECRETARY OF STATE NORTH DAKOTA



[Home](#) | [Business Records Search](#)

PETROLEUM CALIBRATION SERVICE LLC

Corporation Details

System ID: 21146000

Phone: (218) 213-6556

Type: FOREIGN LIMITED LIABILITY COMPANY

Status: Active & Good Standing

Original File Date: 08/01/2005

Effective Date: 08/01/2005

State of Origin: Minnesota

Nature of Business

TEST & CALIBRATE RETAIL MOTOR FUEL DISPENSORS

Principal Office

203 E HIGHWAY 61 ESKO, MN 55733-9610

Registered Agent

BUSINESS FILINGS INCORPORATED

314 E THAYER AVE

BISMARCK, ND 58501-4018

Established Date: Dec 22, 2014

Generate an Annual Report To File

To Generate a Annual Report form to be filed with the Secretary of State, select the appropriate year of the report you intend to file. This report does not contain details of a report previously filed with the Secretary of State. The annual report years reflected are an indication of the various report forms available in this site and is not an indication that an entity needs to file reports for all years. Missing years indicate that the forms for the missing year have not yet been deployed to the website, or have already been removed, and can be obtained by contacting the Secretary of State.


[2014](#) (generates a forms-fillable pdf in a new pop-up window)

[Return to Search Results](#)

[Contact Us](#)

[Disclaimer](#)

[Privacy Policy](#)

 We use Secure Sockets Layer (SSL) encryption technology to ensure your information is secure and protected.

 Will open a new window (pop-up).

W3C WAI AA, CSS, XHTML Compliant | Copyright 2006. All Rights Reserved. The State of North Dakota.



Receipt Date: June 18, 2014
 Test Date: June 24, 2014
 Report Date: June 24, 2014

State Test No.: 332699
 Serial No.: 49433-A
 Bar Code: 201323

Calibration Report

PETROLEUM CALIBRATION SERVICE
 203 E HWY 61
 ESKO, MN 55733
 Contact: GENE LEWIS
 Phone: 218-213-6556
 PO Number: None
 SOP: 32
 Technician ID: 08

Item(s) Submitted: 5 Gallon Prover
 Manufacturer: Seraphin
 Material: ss
 Equipment Number: None
 Condition: Good
 Temperature: 26.°C
 Pressure: 734.9 mmHg
 Relative Humidity: 47. %

Nominal Volume		Error (in ³)	Volume Contained At Zero Line (gallons)	Uncertainty (in ³)	Coefficient of Expansion(°F)
5 gal	As Found	-0.15	4.9994	0.62	0.0000265
	As Left	-0.15	4.9994	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a drain time of 30 seconds after cessation of flow and at a reference temperature of 60°F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.

Results apply to item identified in this report only.

Nils Fleming

Nils Fleming
 Metrologist

Reviewed by:

Mark Nicollet

Mark Nicollet
 Quality Manager



Receipt Date: June 19, 2014
 Test Date: June 24, 2014
 Report Date: June 24, 2014

State Test No.: 332716
 Serial No.: 49433-B
 Bar Code: 202262

Calibration Report

PETROLEUM CALIBRATION SERVICE
 203 E HWY 61
 ESKO, MN 55733
 Contact: GENE LEWIS
 Phone: 218-213-6556
 PO Number: None
 SOP: 32
 Technician ID: 08

Item(s) Submitted: 5 Gallon Measure
 Manufacturer: Seraphin
 Material: ss
 Equipment Number: None
 Condition: Good
 Temperature: 26.°C
 Pressure: 734.9 mmHg
 Relative Humidity: 47. %

Nominal Volume		Error (in ³)	Volume Contained	Uncertainty (in ³)	Coefficient of Expansion(°F)
			At Zero Line (gallons)		
5 gal	As Found	-0.13	4.9994	0.62	0.0000265
	As Left	-0.13	4.9994	0.62	

Neck Calibration: No neck calibration was done at this time.


This measure or prover has been calibrated as a "to contain after wet down" vessel with a drain time of 30 seconds after cessation of flow and at a reference temperature of 60°F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.


Results apply to item identified in this report only.

Nils Fleming

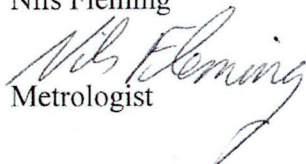
 Metrologist

Reviewed by:

Mark Nicolet


 Quality Manager



Weights & Measures Metrology Laboratory
 14305 Southcross Drive #150
 Burnsville, MN 55306-7008
 651.539.1555 FAX 651.539.1553

Receipt Date: June 18, 2014
 Test Date: June 24, 2014
 Report Date: June 24, 2014

State Test No.: 332700
 Serial No.: 49433-C
 Bar Code: 201324

Calibration Report

PETROLEUM CALIBRATION SERVICE
 203 E HWY 61
 ESKO, MN 55733
 Contact: GENE LEWIS
 Phone: 218-213-6556
 PO Number: None
 SOP: 32
 Technician ID: 08

Item(s) Submitted: 5 Gallon Prover
 Manufacturer: Seraphin
 Material: ss
 Equipment Number: None
 Condition: Good
 Temperature: 26.°C
 Pressure: 734.9 mmHg
 Relative Humidity: 47. %

Nominal Volume		Error (in ³)	Volume Contained At Zero Line (gallons)	Uncertainty (in ³)	Coefficient of Expansion(1/°F)
5 gal	As Found	0.46	5.0020	0.62	0.0000265
	As Left	-0.05	4.9998	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a drain time of 30 seconds after cessation of flow and at a reference temperature of 60°F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.

Results apply to item identified in this report only.

Nils Fleming

 Metrologist

Reviewed by:
 Mark Nicollet

 Quality Manager



Weights & Measures Metrology Laboratory
 14305 Southcross Drive #150
 Burnsville, MN 55306-7008
 651.539.1555 FAX 651.539.1553

Receipt Date: June 18, 2014
 Test Date: June 24, 2014
 Report Date: June 24, 2014

State Test No.: 332701
 Serial No.: 00-13651-15
 Bar Code: 201325

Calibration Report

PETROLEUM CALIBRATION SERVICE
 203 E HWY 61
 ESKO, MN 55733
 Contact: GENE LEWIS
 Phone: 218-213-6556
 PO Number: None
 SOP: 32
 Technician ID: 08

Item(s) Submitted: 5 Gallon Prover
 Manufacturer: Seraphin
 Material: ss
 Equipment Number: None
 Condition: Good
 Temperature: 26.°C
 Pressure: 734.9 mmHg
 Relative Humidity: 47. %

Nominal Volume		Error (in ³)	Volume Contained	Uncertainty (in ³)	Coefficient of Expansion(/°F)
			At Zero Line (gallons)		
5 gal	As Found	-0.15	4.9994	0.62	0.0000265
	As Left	-0.15	4.9994	0.62	

Neck Calibration: No neck calibration was done at this time.


This measure or prover has been calibrated as a "to contain after wet down" vessel with a drain time of 30 seconds after cessation of flow and at a reference temperature of 60°F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.

Results apply to item identified in this report only.


Nils Fleming

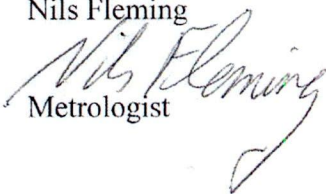

Metrologist

Reviewed by:

Mark Nicollet



Quality Manager

United States Department of Commerce National Institute of Standards and Technology

Certificate of Metrological Traceability For:

Minnesota

This laboratory has demonstrated evidence of an unbroken chain of metrological traceability of its standards to the international system of units (SI), documented measurement uncertainties, uses documented measurement procedures, successfully completed training and proficiency tests, documented calibration intervals, submitted a quality management system, and demonstrated suitable measurement assurance for the Scope listed on this certificate.

The Office of Weights and Measures Program assesses laboratories to NIST Handbook 143 - Program Handbook for State Weights and Measures Laboratories and ISO/IEC 17025:2005.



2014

Scope

Mass Echelon I

30 kg to 1 mg

Mass Echelon II

50 kg to 1 mg
1000 lb to 0.001 lb
4 oz to 0.03125 oz

Mass Echelon III

50 kg to 1 mg
5000 lb to 0.001 lb
8 oz to 0.03125 oz

Weight Carts

10 000 lb to 2000 lb

Wheel Load Weighers

20000 lb to 2000 lb

Railroad Test Cars

110 000 lb to 80 000 lb

Volume Gravimetric, I

20 L to 1 mL
100 gal to 0.25 qt

Volume Transfer, II

1500 gal to 5 gal
100 gal to 25 gal LPG

A handwritten signature in blue ink that reads "Carol T. Hockert".

Carol T. Hockert, Chief
NIST Office of Weights and Measures

Effective Dates: 2014-01-01 to 2014-12-31