



Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334053
Serial No.: 49775
Barcode: 017688

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 32
Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
Manufacturer: Seraphin
Material: Mild Steel
Equipment Number: None
Condition: Fair
Temperature: 19.3 °C
Pressure: 736.4 mmHg
Relative Humidity: 34. %

Nominal Volume		Error (in ³)	Volume Contained	Uncertainty (in ³)	Coefficient of Expansion (°F)
			At Zero Line (gallons)		
5 gal	As Found	0.04	5.0002	0.62	0.0000186
	As Left	0.04	5.0002	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.

Pete Whebbe

Peter J. Whebbe
Metrologist

Reviewed by:
Mark Nicollet

Mark Andrew Nicollet
Quality Manager

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334054
Serial No.: 40961
Barcode: 019293

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 32
Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
Manufacturer: Seraphin
Material: Mild Steel
Equipment Number: None
Condition: Fair/Dirty
Temperature: 19.3 °C
Pressure: 736.4 mmHg
Relative Humidity: 34. %

Nominal Volume		Error (in ³)	Volume Contained At Zero Line (gallons)	Uncertainty (in ³)	Coefficient of Expansion (1/°F)
5 gal	As Found	-1.11	4.9952	0.62	0.0000186
	As Left	0.15	5.0007	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.

Pete Whebbe



Metrologist

Reviewed by:

Mark Nicollet



Quality Manager

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334055
Serial No.: 29726
Barcode: 019891

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 32
Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
Manufacturer: Seraphin
Material: Mild Steel
Equipment Number: None
Condition: Fair/Dirty
Temperature: 19.3 °C
Pressure: 736.4 mmHg
Relative Humidity: 34. %

Nominal Volume		Error (in ³)	Volume Contained	Uncertainty (in ³)	Coefficient of Expansion (1/°F)
			At Zero Line (gallons)		
5 gal	As Found	-0.34	4.9985	0.62	0.0000186
	As Left	-0.09	4.9996	0.62	

Neck Calibration: No neck calibration was done at this time.


This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.


Pete Whebbe



Metrologist

Reviewed by:

Mark Nicollet



Quality Manager

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334056
Serial No.: 42853
Barcode: 019892

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 32
Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
Manufacturer: Seraphin
Material: Mild Steel
Equipment Number: None
Condition: Fair/Dirty
Temperature: 19.3 °C
Pressure: 736.4 mmHg
Relative Humidity: 34. %

Nominal Volume	Error (in ³)	Volume Contained		Uncertainty (in ³)	Coefficient of Expansion (°F)
		At Zero Line	(gallons)		
5 gal	As Found	0.10	5.0004	0.62	0.0000186
	As Left	0.10	5.0004	0.62	

Neck Calibration: No neck calibration was done at this time.


This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.


Pete Whebbe



Metrologist

Reviewed by:

Mark Nicollet



Quality Manager

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334057
Serial No.: 42862
Barcode: 019893

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 32
Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
Manufacturer: Seraphin
Material: Mild Steel
Equipment Number: None
Condition: Fair/Dirty
Temperature: 19.3 °C
Pressure: 736.4 mmHg
Relative Humidity: 34. %

Nominal Volume		Error (in ³)	Volume Contained	Uncertainty (in ³)	Coefficient of Expansion (°F)
			At Zero Line (gallons)		
5 gal	As Found	-0.31	4.9986	0.62	0.0000186
	As Left	-0.01	4.9999	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.


Pete Whebbe



Metrologist

Reviewed by:

Mark Nicollet



Quality Manager

Receipt Date: March 24, 2015
 Test Date: March 25, 2015
 Report Date: March 25, 2015

State Test No.: 334058
 Serial No.: 42886
 Barcode: 019911

Calibration Report

O'DAY EQUIPMENT
 1301 40TH ST NW
 FARGO, ND 58108-2706
 Contact: LYNN STUHAUG
 Phone: 701-282-9260
 PO Number: NONE
 SOP: 32
 Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
 Manufacturer: Seraphin
 Material: Mild Steel
 Equipment Number: None
 Condition: Fair/Dirty
 Temperature: 19.3 °C
 Pressure: 736.4 mmHg
 Relative Humidity: 34. %

Nominal Volume		Error (in ³)	Volume Contained	Uncertainty (in ³)	Coefficient of Expansion (°F)
			At Zero Line (gallons)		
5 gal	As Found	-0.16	4.9993	0.62	0.0000186
	As Left	-0.16	4.9993	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.


Pete Whebbe



Metrologist

Reviewed by:

Mark Nicollet



Quality Manager

Receipt Date: March 24, 2015
 Test Date: March 25, 2015
 Report Date: March 26, 2015

State Test No.: 334060
 Serial No.: 02-52826
 Barcode: 200194

Calibration Report

O'DAY EQUIPMENT
 1301 40TH ST NW
 FARGO, ND 58108-2706
 Contact: LYNN STUHAUG
 Phone: 701-282-9260
 PO Number: NONE
 SOP: 32
 Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
 Manufacturer: Seraphin
 Material: Mild Steel
 Equipment Number: None
 Condition: Fair/Dirty
 Temperature: 19.3 °C
 Pressure: 736.4 mmHg
 Relative Humidity: 34. %

Nominal Volume		Error (in ³)	Volume Contained	Uncertainty (in ³)	Coefficient of Expansion (°F)
			At Zero Line (gallons)		
5 gal	As Found	-0.01	4.9999	0.62	0.0000186
	As Left	-0.01	4.9999	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.

Pete Whebbe

Pete J. Whebbe
 Metrologist

Reviewed by:

Mark Nicollet

Mark Nicollet
 Quality Manager

Receipt Date: March 24, 2015
 Test Date: March 25, 2015
 Report Date: March 26, 2015

State Test No.: 334062
 Serial No.: 09-49760-11
 Barcode: 200945

Calibration Report

O'DAY EQUIPMENT
 1301 40TH ST NW
 FARGO, ND 58108-2706
 Contact: LYNN STUHAUG
 Phone: 701-282-9260
 PO Number: NONE
 SOP: 32
 Technician ID: 11

Item(s) Submitted: 5 Gallon Prover
 Manufacturer: Seraphin
 Material: Stainless Steel
 Equipment Number: None
 Condition: Good
 Temperature: 19.3 °C
 Pressure: 736.4 mmHg
 Relative Humidity: 34. %

Nominal Volume		Error (in ³)	Volume Contained At Zero Line (gallons)	Uncertainty (in ³)	Coefficient of Expansion (°F)
5 gal	As Found	-0.13	4.9994	0.62	0.0000265
	As Left	-0.13	4.9994	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a drain time of 30 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.


Results apply to item identified in this report only.

Pete Whebbe



Metrologist

Reviewed by:
 Mark Nicollet


 Quality Manager

Receipt Date: March 24, 2015
 Test Date: March 25, 2015
 Report Date: March 26, 2015

State Test No.: 334063
 Serial No.: 11-89552
 Barcode: 201818

Calibration Report

O'DAY EQUIPMENT
 1301 40TH ST NW
 FARGO, ND 58108-2706
 Contact: LYNN STUHAUG
 Phone: 701-282-9260
 PO Number: NONE
 SOP: 32
 Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
 Manufacturer: Seraphin
 Material: Stainless Steel
 Equipment Number: None
 Condition: Good
 Temperature: 19.3 °C
 Pressure: 736.4 mmHg
 Relative Humidity: 34. %

Nominal Volume		Error (in ³)	Volume Contained		Coefficient of Expansion (1/°F)
			At Zero Line (gallons)	Uncertainty (in ³)	
5 gal	As Found	-0.56	4.9976	0.62	0.0000265
	As Left	-0.01	5.0000	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.

Pete Whebbe

Pete J. Whebbe
 Metrologist

Reviewed by:

Mark Niccollet

Mark Andrew Niccollet
 Quality Manager

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 26, 2015

State Test No.: 334064
Serial No.: 11-06423
Barcode: 202083

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 32
Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
Manufacturer: Seraphin
Material: Stainless Steel
Equipment Number: None
Condition: Good
Temperature: 19.3 °C
Pressure: 736.4 mmHg
Relative Humidity: 34. %

Nominal Volume	Error (in ³)	Volume Contained		Uncertainty (in ³)	Coefficient of Expansion (°F)
		At Zero Line	(gallons)		
5 gal	As Found	0.04	5.0002	0.62	0.0000265
	As Left	0.04	5.0002	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.

The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.

Pete Whebbe

Metrologist



Reviewed by:

Mark Nicollet

Quality Manager



Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 26, 2015

State Test No.: 334065
Serial No.: 47900
Barcode: 202097

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 32
Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
Manufacturer: Seraphin
Material: Mild Steel
Equipment Number: None
Condition: Fair/Dirty
Temperature: 19.3 °C
Pressure: 736.4 mmHg
Relative Humidity: 34. %

Nominal Volume	Error (in ³)	Volume Contained		Uncertainty (in ³)	Coefficient of Expansion (°F)
		At Zero Line (gallons)			
5 gal	As Found	0.01	5.0000	0.62	0.0000186
	As Left	0.01	5.0000	0.62	

Neck Calibration: No neck calibration was done at this time.

This measure or prover has been calibrated as a "to contain after wet down" vessel with a pour time of 30 seconds, a drain time of 10 seconds after cessation of full flow and at a reference temperature of 60 °F.


The measure or prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.

Pete Whebbe

Metrologist

Reviewed by:
Mark Nicollet

Quality Manager

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 26, 2015

State Test No.: 334061
Serial No.: 06-03229
Barcode: 200458

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 32
Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
Manufacturer: Seraphin
Material: Stainless Steel
Equipment Number: None
Condition: Leaks
Temperature: 19.3 °C
Pressure: 736.4 mmHg
Relative Humidity: 34. %

Nominal Volume	Error (in ³)	Volume Contained		Coefficient of Expansion (°F)
		At Zero Line (gallons)	Uncertainty (in ³)	

Measure is **REJECTED**. Leaks from weld at base of sight tube.


Pete Whebbe



Metrologist

Reviewed by:

Mark Nicollet



Quality Manager

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334059
Serial No.: 42840
Barcode: 200167

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 32
Technician ID: 11

Item(s) Submitted: 5 Gallon Measure
Manufacturer: Seraphin
Material: Mild Steel
Equipment Number: None
Condition: Leaks
Temperature: 19.3 °C
Pressure: 736.4 mmHg
Relative Humidity: 34. %

Nominal Volume	Error (in ³)	Volume Contained		Coefficient of Expansion (°F)
		At Zero Line (gallons)	Uncertainty (in ³)	

Measure is **REJECTED**. Leaks at base of neck.

Pete Whebbe


Metrologist



Reviewed by:

Mark Niccollet

Quality Manager

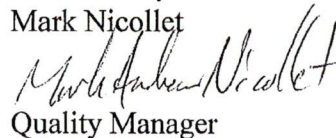

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334052
Serial No.: 103
Barcode: 018789

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706

Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 33
Technician ID: 07

Item(s) Submitted: 100 Gallon Prover
Manufacturer: KLEESPIE
Material: Mild Steel
Description: Dry Bottom
Condition: Fair
Temperature: 18.8°C
Pressure: 735. mmHg
Relative Humidity: 37. %

Nominal Volume		Volume (gallons)	Error (in ³)	Uncertainty (in ³)	Coefficient of Expansion(°F)
100 gal	As Found	100.006	1.3	3.0	0.0000186
	As Left	100.006	1.3	3.0	

Neck Calibration: No neck calibration was done at this time.


This prover has been calibrated as a "to contain after wet down" vessel with a drain time of 30 seconds after cessation of full flow and at a reference temperature of 60 °F.

The prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.


Mark Nicollet



Quality Manager

Reviewed by:

Pete Whebbe



Metrologist

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334051
Serial No.: 3758
Barcode: 019923

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706

Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 33
Technician ID: 07

Item(s) Submitted: 100 Gallon Prover
Manufacturer: Unknown
Material: Mild Steel
Description: Dry Bottom
Condition: Good
Temperature: 18.7°C
Pressure: 735.6 mmHg
Relative Humidity: 38. %

Nominal Volume		Volume (gallons)	Error (in ³)	Uncertainty (in ³)	Coefficient of Expansion(/°F)
100 gal	As Found	100.008	1.8	3.0	0.0000186
	As Left	100.008	1.8	3.0	

Neck Calibration: No neck calibration was done at this time.

This prover has been calibrated as a "to contain after wet down" vessel with a drain time of 30 seconds after cessation of full flow and at a reference temperature of 60 °F.

The prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95 %.

Results apply to item identified in this report only.


Mark Nicollet



Quality Manager

Reviewed by:

Pete Whebbe



Metrologist

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334050
Serial No.: 12640
Barcode: 019910

Calibration Report

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 34
Technician ID: 07

Item(s) Submitted: 100 gallon LPG Prover
Manufacturer: Arrow Tank
Material: Mild Steel
Description: Wet Bottom
Condition: Good
Temperature: 18.4°C
Pressure: 737.4 mmHg
Relative Humidity: 30. %

Nominal Volume	Error As Found (in ³)	Error As Left (in ³)	Uncertainty (in ³)	Coefficient of Expansion(/°F)
100 gal	-11	-11	10	0.0000186

Neck Calibration: No neck calibration was done at this time.


This prover has been calibrated as a "to contain after wet down" vessel at a reference temperature of 60 °F and a reference pressure of 100 psig.

The prover listed above has been compared by volumetric transfer methods to the standards of the State of Minnesota. The standards are traceable to the SI through NIST. Statistical process control charts indicate standards are currently in control. All gauges were sealed in place.

The reported uncertainty conforms to NIST Technical Note 1297. The confidence interval is 95%.

Results apply to item identified in this report only.


Mark Nicollet



Quality Manager

Reviewed by:

Pete Whebbe



Metrologist

Receipt Date: March 24, 2015
Test Date: March 25, 2015
Report Date: March 25, 2015

State Test No.: 334050
Serial No.: 12640
Barcode: 019910

Pressure Correction Chart

O'DAY EQUIPMENT
1301 40TH ST NW
FARGO, ND 58108-2706
Contact: LYNN STUHAUG
Phone: 701-282-9260
PO Number: NONE
SOP: 34
Technician ID: 07

Item(s) Submitted: 100 gallon LPG Prover
Manufacturer: Arrow Tank
Material: Mild Steel
Description: Wet Bottom
Condition: Good
Temperature: 18.4°C
Pressure: 737.4 mmHg
Relative Humidity: 30. %

Pressure Gauge Reading (PSIG)	Volume Correction (gal)
0	-0.181
10	-0.165
20	-0.148
30	-0.132
40	-0.115
50	-0.099
60	-0.088
70	-0.078
80	-0.067
90	-0.057
100	-0.046
110	-0.040
120	-0.034
130	-0.028
140	-0.022
150	-0.016
160	-0.008
170	0.001
180	0.009
190	0.018
200	0.026

Mark Nicollet



Quality Manager