



APPLICATION FOR REGISTRATION AS A REGISTERED SERVICE COMPANY

Public Service Commission
SFN 51277 (2/2014)



TYPE OR PRINT - AN INCOMPLETE OR ILLEGIBLE APPLICATION WILL BE REJECTED

Name of Company Midwest Meter Provers Allen Marsolek	Email Address	Application Date 4-10-15	
Mailing Address 2965 85th Ave S, E,	City Jamestown	State N.D.	Zip Code 58401
Telephone Number	Cell Phone Number 701-320-3698	Fax Number	

Select below all device types your company will certify:

Scales (include maximum capacity, if applicable)	Liquid (include maximum flow rate, if applicable)
<input type="checkbox"/> 1. Rail <input type="checkbox"/> 2. Truck <input type="checkbox"/> 3. Livestock <input type="checkbox"/> 4. Hopper: Max. Capacity: _____ <input type="checkbox"/> 5. Belt <input checked="" type="checkbox"/> 6. Over 30 lbs.: Max. Capacity: <u>3000 Lbs</u> <input type="checkbox"/> 7. 30 lbs. or less <input type="checkbox"/> 8. Class II (indicate on your calibration report which weight kit is Class II certified) <input type="checkbox"/> 9. Other: Please List:	<input type="checkbox"/> 1. Retail Fuel (less than 20 gal. per minute) <input type="checkbox"/> 2. High Flow Retail Fuel (20 gal. per minute or greater) <input type="checkbox"/> 3. Vehicle Tank: Max. Flow Rate: _____ <input type="checkbox"/> 4. Stationary Bulk (fuel or oil): Max. Flow Rate: _____ <input type="checkbox"/> 5. LPG <input type="checkbox"/> 6. Stationary LPG <input type="checkbox"/> 7. Fertilizer: Max. Flow Rate: _____ <input type="checkbox"/> 8. Chemical <input type="checkbox"/> 9. Anhydrous <input type="checkbox"/> 10. Loading Rack <input type="checkbox"/> 11. Other: Please List:

List below all persons employed by your company as a North Dakota Registered Service Person and the device types they are registered to certify (attach a separate sheet to list additional employees):

Permit No.	Employee	Device Types Registered to Certify (list using device type numbers from above)
e.g. 1001	e.g. John Doe	e.g. Scales - 2, 3, 6, 8; e.g. Liquid - 1, 2, 6
1503	Allen Marsolek	Scale 6

Continued on Page 2

2 WM-15-78 Filed: 4/15/2015 Pages: 7
Application for permit
Midwest Meter Prover's

Application for Registration as a Registered Service Company
Page 2



List below all field standards (attach current calibration reports):

Additional Application Items (initial where appropriate):

Standardized Test Report	<input checked="" type="checkbox"/> Copy enclosed <input type="checkbox"/> No change in report filed previously
Tested and Approved Sticker	<input checked="" type="checkbox"/> Copy enclosed <input type="checkbox"/> No change in sticker filed previously
Photocopy of Crimped Lead Wire Seal	<input checked="" type="checkbox"/> Copy enclosed <input type="checkbox"/> No change in crimped lead wire seal filed previously

per conversation with Allen Marsolek on 5-12-15 - no change in items previously filed
BB

Public Company Listing:


Include my company information on your registered service company list for public contact.
 Yes No

I am Allen Marsolek, and have authority to represent this company. By signing this application, I declare that I have examined this form and accompanying documentation, and to the best of my knowledge and belief, the facts stated and documentation provided is true, correct, and complete.


Allen Marsolek
Signature

Send Completed Application and Related Documents To:
Public Service Commission
600 E Boulevard Ave Dept 408
Bismarck ND 58505-0480
Telephone: (701) 328-2400
Fax: (701) 328-2410

North Dakota

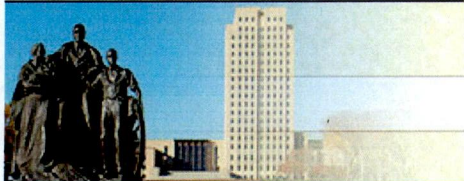nd.gov Official Portal for
North Dakota State GovernmentNorth Dakota
LEGENDARY

SECRETARY OF STATE NORTH DAKOTA

[Home](#) | [Business Records Search](#)

MIDWEST METER PROVER'S

Trade Name

System ID: 13488600**Phone:** Not on file**Status:** Active**Original File Date:** 04/17/1998**Last Renewal Date:** 04/17/2013

Nature of Business

TEST ANHYDROUS METERS IN THE STATE OF NORTH DAKOTA; THESE TESTS DETERMINE THAT THE CUSTOMER IS RECEIVING THE APPROPRIATE AMOUNT OF PRODUCT


Owners

ALLEN MARSOLEK

2965 85TH AVE SE


JAMESTOWN, ND 58401-9604

[Return to Search Results](#)[Contact Us](#)[Disclaimer](#)[Privacy Policy](#)

 We use Secure Sockets Layer (SSL) encryption technology to ensure your information is secure and protected.

 Will open a new window (pop-up).

W3C WAI AA, CSS, XHTML Compliant | Copyright 2006. All Rights Reserved. The State of North Dakota.

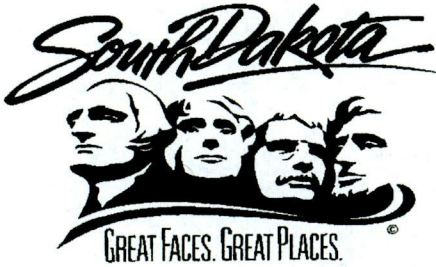

**SOUTH DAKOTA
DEPARTMENT OF PUBLIC SAFETY**

**Office of Weights and Measures
Metrology Lab**

Lab: 1500 N Garfield – E. Truck Bypass Phone: 605-773-3170
Office: 118 West Capitol Avenue Phone: 605-773-3697

REPORT OF CALIBRATION

**LAB TEST NUMBER: MP3379
DATE OF REPORT: 04/10/2015
DATE RECEIVED: 04/10/2015
DATE OF TEST: 04/10/2015**



Submitted By: Midwest Meter Provers
Contact: Alan Marsolek
Mailing Address: 2965 85th Ave SE
City, State, Zip: Jamestown, ND 58401
Phone: 701-320-3698
S/A Number:

Standards Submitted:

1 -Truck Scale

Uncertainty Statement: The combined standard uncertainty includes the standard uncertainty reported for the standard, the standard uncertainty for the measurement process, and a component of uncertainty to account for any observed deviations from values that are less than surveillance limits. The combined standard uncertainty is multiplied by a coverage factor k to provide an expanded uncertainty, which defines an interval having a level of confidence of approximately 95 percent. The expanded uncertainty presented in this report is consistent with the ISO/IEC Guide to the Expression of Uncertainty in Measurement. The expanded uncertainty is not to be confused with a tolerance limit for the user during application. All established Uncertainties are less than 1/3 applicable Class "F" tolerances.

Traceability statement:


The Standards of the SD Metrology Laboratory are traceable to the International System of Units (SI) through the National Institute of Standards and Technology. The laboratory test number identified above is the unique report number to be used in referencing measurement traceability for artifacts identified in this report only.

The artifacts submitted for calibration have been examined by the State of South Dakota and found to be appropriate for the intended use and to be accurate within Class "F" Tolerances as established by the National Institute of Standards and Technology-Weights and Measures Division. Test methods are in accordance with NIST Handbook 145 and NIST IR 6969 and/or NIST IR 7383.

This document does not represent or imply endorsement by NIST Office of Weights and Measures, NMI, or any agency of the State and/or national governments. The reported test values relate only to the observations made at the time and conditions of the test. This report may not be reproduced, except in full without the written approval of this laboratory. The client must not use this document to claim product endorsement by this laboratory.


Ron Peterson, Metrologist




Date

SOUTH DAKOTA WEIGHTS AND MEASURES / METROLOGY LAB

Lab: 1500 N. Garfield-E. Truck Bypass Phone: 605-773-3170

Office: 118 West Capitol Avenue Phone: 605-773-3697

Pierre, SD 57501

Submitted by :	ALLAN MARSOLEK	Report Number:	MP3379
Mailing Address:	2965 85 th Ave SE	Date Received:	04/10/15
City, State, Zip:	Jamestown, ND 58401	Date Tested:	04/10/15
Make of Scale:	Rice Lake	Condition of Scale:	Good
Serial Number:	0008689	Temperature (c):	21
Capacity:	3000 lb X 0.5 lb	Humidity:	40.0%
		Pressure (mm/Hg):	716.6

Test Load (lb)	As Found (lb)	Error (lb)	Allowable Tolerance (+/- lb)	PASS/FAIL	As Left (lb)	Error (lb)
0	0	0	0.5	P	0	0
500	500	0	0.5	P	499.5	-0.5
1000	999.5	-0.5	1.0	P	1000.0	0
1500	1498.5	-1.5	1.5	P	1500.0	0

A shift test was performed using 1000 lb standard and the results fell within tolerance.


Repeatability test was performed and scale repeated within tolerance requirements.

A sensitivity weight of 5 lb was used at each weight and the results were within tolerance.

Standards used were calibrated using the working standards of the SD Metrology lab which were tested by the Minnesota State Lab, Report #332339, on 04/03/14 and are traceable to NIST.




END OF REPORT


 Ron Peterson, Metrologist
 Office of Weights and Measures
 118 W Capitol
 Pierre, SD 57501-2000

04/10/15
 Date
 Phone: 605-773-3697
 FAX: 605-773-6131
www.state.sd.us/dps/wm



RECEIVED
APR 15 2015
ND Public
Service
Commission

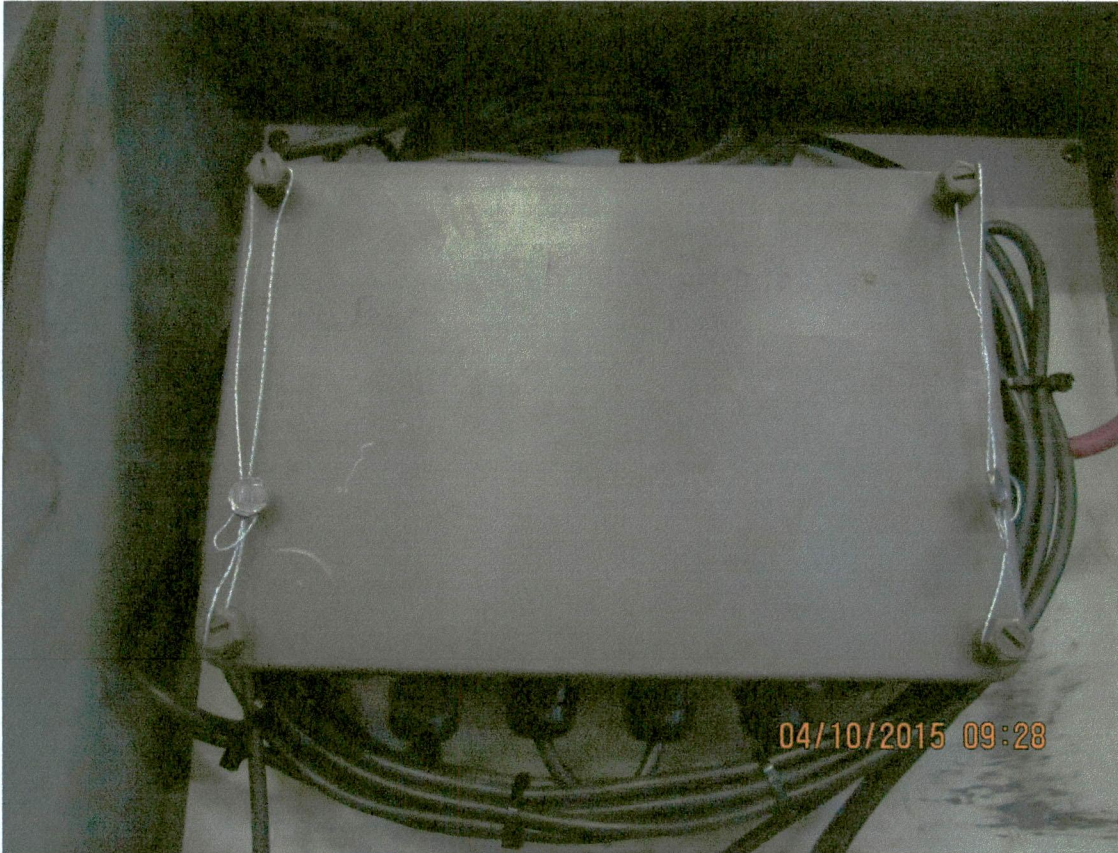

United States Department of Commerce

National Institute of Standards and Technology

Certificate of Metrological Traceability For:

South Dakota

This laboratory has demonstrated evidence of an unbroken chain of metrological traceability of its standards to the international system of units (SI), documented measurement uncertainties, uses documented measurement procedures, successfully completed training and proficiency tests, documented calibration intervals, submitted a quality management system, and demonstrated suitable measurement assurance for the Scope listed on this certificate.

The Office of Weights and Measures Program assesses laboratories to NIST Handbook 143 - Program Handbook for State Weights and Measures Laboratories and ISO/IEC 17025:2005.

Scope

Mass Echelon III

30 kg to 50 mg
1000 lb to 0.001 lb
8 oz to 0.03125 oz

Weight Carts

5000 lb to 2000 lb

Volume Transfer, II

5 gal



2015

A handwritten signature in blue ink, reading "Carol T. Hockert".

Carol T. Hockert, Chief
NIST Office of Weights and Measures

Effective Dates: 2015-01-01 to 2015-12-31