



APPLICATION FOR REGISTRATION AS A REGISTERED SERVICE COMPANY

Public Service Commission
SFN 51277 (2/2014)



TYPE OR PRINT - AN INCOMPLETE OR ILLEGIBLE APPLICATION WILL BE REJECTED

Name of Company CLOVERDALE FOODS COMPANY	Email Address GENEK @ CLOVERDALE FOODS.COM	Application Date 20 DEC 16	
Mailing Address 3015 34TH ST NW	City MANDAN	State ND	Zip Code 58554
Telephone Number (701) 663-9511	Cell Phone Number (701) 202-1042	Fax Number (701) 663-0690	

Select below all device types your company will certify:

Scales (include maximum capacity, if applicable)	Liquid (include maximum flow rate, if applicable)
<input type="checkbox"/> 1. Rail <input type="checkbox"/> 2. Truck <input type="checkbox"/> 3. Livestock <input type="checkbox"/> 4. Hopper: Max. Capacity: _____ <input checked="" type="checkbox"/> 5. Belt <input checked="" type="checkbox"/> 6. Over 30 lbs.: Max. Capacity: 100 <input checked="" type="checkbox"/> 7. 30 lbs. or less <input type="checkbox"/> 8. Class II (indicate on your calibration report which weight kit is Class II certified) <input type="checkbox"/> 9. Other: Please List:	<input type="checkbox"/> 1. Retail Fuel (less than 20 gal. per minute) <input type="checkbox"/> 2. High Flow Retail Fuel (20 gal. per minute or greater) <input type="checkbox"/> 3. Vehicle Tank: Max. Flow Rate: _____ <input type="checkbox"/> 4. Stationary Bulk (fuel or oil): Max. Flow Rate: _____ <input type="checkbox"/> 5. LPG <input type="checkbox"/> 6. Stationary LPG <input type="checkbox"/> 7. Fertilizer: Max. Flow Rate: _____ <input type="checkbox"/> 8. Chemical <input type="checkbox"/> 9. Anhydrous <input type="checkbox"/> 10. Loading Rack <input type="checkbox"/> 11. Other: Please List:

List below all persons employed by your company as a North Dakota Registered Service Person and the device types they are registered to certify (attach a separate sheet to list additional employees):

Permit No.	Employee	Device Types Registered to Certify (list using device type numbers from above)
e.g. 1001	e.g. John Doe	e.g. Scales - 2, 3, 6, 8; e.g. Liquid - 1, 2, 6
1795	EUGENE KELLER	5, 6, 7

Continued on Page 2

2

WM-16-703 Filed: 12/20/2016 Pages: 10
Application for permit

Cloverdale Foods Company



List below all field standards (attach current calibration reports):

500 #	2	
50 #	3	
20 #	6	
10 #	8	
5 #	11	
2 #	7	
1 #	8	
1/2 # (8oz)	2	
4 oz	1	


Additional Application Items (initial where appropriate):

Standardized Test Report	<input checked="" type="checkbox"/> Copy enclosed <input checked="" type="checkbox"/> No change in report filed previously
Tested and Approved Sticker	<input type="checkbox"/> Copy enclosed <input type="checkbox"/> No change in sticker filed previously
Photocopy of Crimped Lead Wire Seal	<input checked="" type="checkbox"/> Copy enclosed <input checked="" type="checkbox"/> No change in crimped lead wire seal filed previously

Public Company Listing:

Include my company information on your registered service company list for public contact.
 Yes No

I am EUGENE KELLER, and have authority to represent this company.
By signing this application, I declare that I have examined this form and accompanying documentation, and to the best of my knowledge and belief, the facts stated and documentation provided is true, correct, and complete.

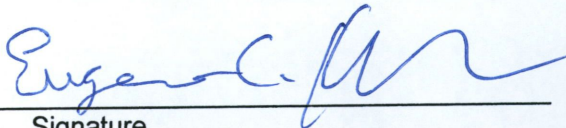


Signature

Send Completed Application and Related Documents To:

Public Service Commission
600 E Boulevard Ave Dept 408
Bismarck ND 58505-0480
Telephone: (701) 328-2400
Fax: (701) 328-2410

North Dakota

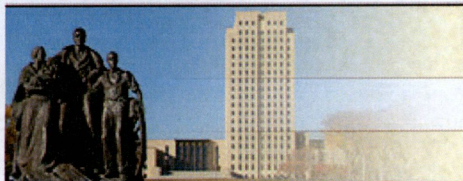nd.gov Official Portal for
North Dakota State GovernmentNorth Dakota
LEGISLATURE

SECRETARY OF STATE NORTH DAKOTA


[Home](#) | [Business Records Search](#)

CLOVERDALE FOODS COMPANY

Corporation Details

System ID: 1632000 **Phone:** (701) 663-9511
Type: BUSINESS CORPORATION
Status: Active & Good Standing
Original File Date: 09/12/1925 **Effective Date:** 09/12/1925
State of Origin: North Dakota

Nature of Business

FOOD MANUFACTURING

Principal Office

3015 34TH ST NW PO BOX 667 MANDAN, ND 58554-0667

Registered Agent

T J RUSSELL
 3015 34TH ST NW
 PO BOX 667
 MANDAN, ND 58554-0667
 Established Date: Jul 07, 2000

Authorized Shares

Class	Number	Par Value
COMMON	100.000000	\$5000.000000

Generate an Annual Report To File

To Generate a Annual Report form to be filed with the Secretary of State, select the appropriate year of the report you intend to file. This report does not contain details of a report previously filed with the Secretary of State. The annual report years reflected are an indication of the various report forms available in this site and is not an indication that an entity needs to file reports for all years. Missing years indicate that the forms for the missing year have not yet been deployed to the website, or have already been removed, and can be obtained by contacting the Secretary of State.

[2016](#) (generates a forms-fillable pdf in a new pop-up window)

[Return to Search Results](#)

[Contact Us](#)
[Disclaimer](#) | [Privacy Policy](#)

We use Secure Sockets Layer (SSL) encryption technology to ensure your information is secure and protected.

Will open a new window (pop-up).

W3C WAI AA, CSS, XHTML Compliant | Copyright 2006. All Rights Reserved. The State of North Dakota.



Receipt Date: February 29, 2016
Test Date: March 2, 2016
Report Date: March 2, 2016

State Test No.: 335634
Set Serial No.: None
Barcode: 201064

Calibration Report

CLOVERDALE FOODS COMPANY
3015 34TH ST NW
MANDAN, ND 58554
Contact: LARRY HUETHER
Phone: 701-667-8512
PO Number: NONE
SOP: 12
Technician ID: 11

Item(s) Submitted: Cast Cube Weights
Manufacturer: Rice Lake
ASTM E617 Type: II
Equipment ID#: None
Condition: Good
Temperature: 19.2 °C
Pressure: 736.5 mmHg
Relative Humidity: 48.4 %

Nominal Value	Serial No.	Correction (g)		NIST HB105-1 Class		Uncertainty (g) (k = 2)
		As Found	As Left	As Found	As Left	
500 lb	Short	-14.7	-14.7	F	F	1.6
500 lb	Tall	22.2	1.2	*	F	1.6

* Weight(s) as found exceed NIST HB 105-1 Class F tolerance.

When used as a set these weights meet NIST HB 105-1 Class F tolerances.

The resulting tolerance class of the weight is determined by combining the correction of the weight and the uncertainty of the measurement. The corrections given above correlate to a conventional mass scale versus 8.0 g/cm³ density and an air density of 1.2 mg/cm³. The items listed above have been compared to the Standards of the State of Minnesota which are currently in control. These standards are traceable to the SI through NIST. Calibration processes were monitored and found to be in control. All of the tolerances and specifications were evaluated according to NIST Handbook 105-1 (1990). Uncertainty calculations contain the components in NIST SOP 8 and conform to the ISO/IEC Guide to the Expression of Uncertainty in Measurement (2008). Results apply to items identified in this report only.

Pete Whebbe

Metrologist

Reviewed by:

Mark Nicollet

Quality Manager



Receipt Date: March 1, 2016
Test Date: March 3, 2016
Report Date: March 3, 2016

State Test No.: 335635
Set Serial No.: None
Barcode: 201065

Calibration Report

CLOVERDALE FOODS COMPANY
3015 34TH ST NW
MANDAN, ND 58554

Contact: Larry Huether
Phone: 701-667-8512
PO Number: None
SOP: 12
Technician ID: 19


Item(s) Submitted: 50 lb, 20 lb Hand Weights
Manufacturer: Rice Lake
ASTM E617 Type: II
Equipment ID#: None
Condition: Good
Temperature: 19.1 °C
Pressure: 740.4 mmHg
Relative Humidity: 50.0 %

Nominal Value	Serial No.	Correction (mg)		NIST HB105-1 Class		Uncertainty (mg) (k = 2)
		As Found	As Left	As Found	As Left	
50 lb		1530	1530	F	F	120
50 lb		920	920	F	F	120
50 lb		930	930	F	F	120
20 lb		120	120	F	F	67
20 lb		-150	-150	F	F	67
20 lb		220	220	F	F	67
20 lb		630	630	F	F	67
20 lb		430	430	F	F	67
20 lb		70	70	F	F	67

When used as a set these weights meet NIST HB 105-1 Class F tolerances.

The resulting tolerance class of the weight is determined by combining the correction of the weight and the uncertainty of the measurement. The corrections given above correlate to a conventional mass scale versus 8.0 g/cm³ density and an air density of 1.2 mg/cm³. The items listed above have been compared to the Standards of the State of Minnesota which are currently in control. These standards are traceable to the SI through NIST. Calibration processes were monitored and found to be in control. All of the tolerances and specifications were evaluated according to NIST Handbook 105-1 (1990). Uncertainty calculations contain the components in NIST SOP 8 and conform to the ISO/IEC Guide to the Expression of Uncertainty in Measurement (2008). Results apply to items identified in this report only.


Erik Alfvin



Metrologist

Reviewed by:

Mark Nicollet



Quality Manager



Receipt Date: March 1, 2016
Test Date: March 2, 2016
Report Date: March 2, 2016

State Test No.: 335636
Set Serial No.: NONE & INDIVIDUAL
Barcode: 201078

Calibration Report

CLOVERDALE FOODS COMPANY
3015 34TH ST NW
MANDAN, ND 58554

Contact: Larry Huether
Phone: 701-667-8512
PO Number: None
SOP: 12
Technician ID: 19

Item(s) Submitted: AVDP Weights - F
Manufacturer: Rice Lake
ASTM E617 Type: II
Equipment ID#: None
Condition: Good
Temperature: 20.6 °C
Pressure: 736.7 mmHg
Relative Humidity: 48.6 %

Nominal Value	Serial No.	Correction (mg)		NIST HB105-1 Class		Uncertainty (mg) (k = 2)
		As Found	As Left	As Found	As Left	
5 lb		-1	-1	F	F	12
5 lb		-21	-21	F	F	12
2 lb		42.1	42.1	F	F	4.8
2 lb		-17.0	-17.0	F	F	4.8
2 lb	0161	42.9	42.9	F	F	4.8
2 lb	6355	35.7	35.7	F	F	4.8

When used as a set these weights meet NIST HB 105-1 Class F tolerances.

The resulting tolerance class of the weight is determined by combining the correction of the weight and the uncertainty of the measurement. The corrections given above correlate to a conventional mass scale versus 8.0 g/cm³ density and an air density of 1.2 mg/cm³. The items listed above have been compared to the Standards of the State of Minnesota which are currently in control. These standards are traceable to the SI through NIST. Calibration processes were monitored and found to be in control. All of the tolerances and specifications were evaluated according to NIST Handbook 105-1 (1990). Uncertainty calculations contain the components in NIST SOP 8 and conform to the ISO/IEC Guide to the Expression of Uncertainty in Measurement (2008). Results apply to items identified in this report only.

Erik Alfvin

Metrologist

Reviewed by:

Mark Nicollet

Quality Manager



Receipt Date: March 11, 2016
Test Date: March 15, 2016
Report Date: March 16, 2016

State Test No.: 335684
Set Serial No.: 1/NONE
Barcode: 201752

Calibration Report

CLOVERDALE FOODS COMPANY
3015 34TH ST NW
MANDAN, ND 58554
Contact: LARRY HUETHER
Phone: 701-667-8512
PO Number: NONE
SOP: 12
Technician ID: 9

Item(s) Submitted: Satin stainless weights
Manufacturer: Rice Lake
ASTM E617 Type: II
Equipment ID#: None
Condition: Fair
Temperature: 20.5 °C
Pressure: 726.5 mmHg
Relative Humidity: 47.9 %

Nominal Value	lb	Serial No.	Correction (mg)		ASTM E617 Class		Uncertainty (mg) (k = 2)
			As Found	As Left	As Found	As Left	
10	lb		10.	10.	4	4	15
10	lb		-82	-82	5	5	15
10	lb		-148	-148	6	6	15
5	lb	1	60.	60.	5	5	12
5	lb		1.0	1.0	4	4	12
5	lb		24	24	4	4	12
5	lb		23	23	4	4	12
5	lb		16	16	4	4	12
2	lb		6.9	6.9	5	5	4.8
2	lb		25.1	25.1	5	5	4.8
1	lb		-14.7	-14.7	5	5	2.8
1	lb		16.1	16.1	5	5	2.8
0.5	lb		1.6	1.6	4	4	2.3

The resulting tolerance class of the weight is determined by combining the correction of the weight and the uncertainty of the measurement. The corrections given above correlate to a conventional mass scale versus 8.0 g/cm³ density and an air density of 1.2 mg/cm³. The items listed above have been compared to the Standards of the State of Minnesota which are currently in control. These standards are traceable to the SI through NIST. Calibration processes were monitored and found to be in control. All of the tolerances and specifications were evaluated according to ASTM E617 (2013). Uncertainty calculations contain the components in NIST SOP 8 and conform to the ISO/IEC Guide to the Expression of Uncertainty in Measurement (2008). Results apply to items identified in this report only.

Heidi Jones
Heidi Jones
Laboratory Administrator

Reviewed by:
Mark Nicollet
Mark Nicollet
Quality Manager





Receipt Date: February 29, 2016
Test Date: March 2, 2016
Report Date: March 2, 2016

State Test No.: 335633
Set Serial No.: None/Loose Weights
Barcode: 201059

Calibration Report

CLOVERDALE FOODS COMPANY
3015 34TH ST NW
MANDAN, ND 58554

Contact: Larry Huether
Phone: 701-667-8512
PO Number: None
SOP: 12
Technician ID: 19

Item(s) Submitted: AVDP Weight Kit - F
Manufacturer: Rice Lake, Troemner
ASTM E617 Type: II
Equipment ID#: None
Condition: Good
Temperature: 20.5 °C
Pressure: 736.9 mmHg
Relative Humidity: 48.3 %

Nominal Value	Serial No.	Correction (mg)		NIST HB105-1 Class		Uncertainty (mg) (k = 2)
		As Found	As Left	As Found	As Left	
10 .. lb		81	81	F	F	15
10 lb	2	113	113	F	F	15
10 lb	3	133	133	F	F	15
5 . lb		44	44	F	F	12
5 .. lb		34	34	F	F	12
5 lb	2	-1	-1	F	F	12
1 . lb		24.0	24.0	F	F	2.8
1 .. lb		19.0	19.0	F	F	2.8
1 lb	2	24.6	24.6	F	F	2.8
1 lb	0480	47.2	47.2	F	F	2.8
1 lb	0487	22.3	22.3	F	F	2.8
8 oz		-12.2	-12.2	F	F	2.3
4 oz	3	6.57	6.57	F	F	0.60

When used as a set these weights meet NIST HB 105-1 Class F tolerances.

The resulting tolerance class of the weight is determined by combining the correction of the weight and the uncertainty of the measurement. The corrections given above correlate to a conventional mass scale versus 8.0 g/cm³ density and an air density of 1.2 mg/cm³. The items listed above have been compared to the Standards of the State of Minnesota which are currently in control. These standards are traceable to the SI through NIST. Calibration processes were monitored and found to be in control. All of the tolerances and specifications were evaluated according to NIST Handbook 105-1 (1990). Uncertainty calculations contain the components in NIST SOP 8 and conform to the ISO/IEC Guide to the Expression of Uncertainty in Measurement (2008). Results apply to items identified in this report only.

Erik Alfvín

Metrologist

Reviewed by:

Mark Nicollet

Quality Manager





Receipt Date: February 29, 2016
Test Date: March 2, 2016
Report Date: March 2, 2016

State Test No.: 335632
Set Serial No.: None
Barcode: 202016

Calibration Report

CLOVERDALE FOODS COMPANY
3015 34TH ST NW
MANDAN, ND 58554

Contact: Larry Huether
Phone: 701-667-8512
PO Number: None
SOP: 12
Technician ID: 19

Item(s) Submitted: AVDP Weight Kit - F
Manufacturer: Rice Lake
ASTM E617 Type: II
Equipment ID#: None
Condition: Good
Temperature: 20.7 °C
Pressure: 736.7 mmHg
Relative Humidity: 50.0 %

Nominal Value	Serial No.	Correction (mg)		NIST HB105-1 Class		Uncertainty (mg) (k = 2)
		As Found	As Left	As Found	As Left	
10 lb	1	117	117	F	F	15
10 lb		93	93	F	F	15
5 lb		55	55	F	F	12
2 lb		35.0	35.0	F	F	4.8
1 lb		17.5	17.5	F	F	2.8

When used as a set these weights meet NIST HB 105-1 Class F tolerances.

The resulting tolerance class of the weight is determined by combining the correction of the weight and the uncertainty of the measurement. The corrections given above correlate to a conventional mass scale versus 8.0 g/cm³ density and an air density of 1.2 mg/cm³. The items listed above have been compared to the Standards of the State of Minnesota which are currently in control. These standards are traceable to the SI through NIST. Calibration processes were monitored and found to be in control. All of the tolerances and specifications were evaluated according to NIST Handbook 105-1 (1990). Uncertainty calculations contain the components in NIST SOP 8 and conform to the ISO/IEC Guide to the Expression of Uncertainty in Measurement (2008). Results apply to items identified in this report only.

Erik Alfvín
Erik Alfvín

Metrologist

Reviewed by:
Mark Nicollet
Mark Nicollet
Quality Manager

United States Department of Commerce National Institute of Standards and Technology

Certificate of Metrological Traceability For:

Minnesota

This laboratory has demonstrated evidence of an unbroken chain of metrological traceability of its standards to the international system of units (SI), documented measurement uncertainties, uses documented measurement procedures, successfully completed training and proficiency tests, documented calibration intervals, submitted a quality management system, and demonstrated suitable measurement assurance for the Scope listed on this certificate.

The Office of Weights and Measures Program assesses laboratories to NIST Handbook 143 - Program Handbook for State Weights and Measures Laboratories and ISO/IEC 17025:2005.

Scope

Mass Echelon II
50 kg to 1 mg
1000 lb to 0.001 lb
4 oz to 0.03125 oz

Mass Echelon III
50 kg to 1 mg
5000 lb to 0.001 lb
4 oz to 0.03125 oz


Weight Carts
10 000 lb to 2000 lb

Wheel Load Weighers
20 000 lb to 2000 lb

Railroad Test Cars
110 000 lb to 80 000 lb

Volume Gravimetric, I
20 L to 10 mL
100 gal to 0.25 qt

Volume Transfer, II
1500 gal to 5 gal
100 gal to 25 gal LPG

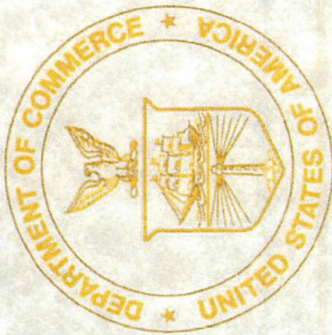

2016 to 2017

Carol T. Hockett, Chief
NIST Office of Weights and Measures

Effective Dates: 2016-01-01 to 2017-12-31