



**APPLICATION FOR REGISTRATION AS A REGISTERED SERVICE COMPANY**  
 Public Service Commission  
 SFN 51277 (2/2014)



TYPE OR PRINT - AN INCOMPLETE OR ILLEGIBLE APPLICATION WILL BE REJECTED

Name of Company <i>CompuCom</i>	Email Address <i>Penni.Beall@compucom.com</i>	Application Date <i>12/6/16</i>	
Mailing Address <i>8383 Dominion Pkwy</i>	City <i>Plano</i>	State <i>TX</i>	Zip Code <i>75024</i>
Telephone Number <i>972-856-3850</i>	Cell Phone Number	Fax Number	

Select below all device types your company will certify:

Scales (include maximum capacity, if applicable)	Liquid (include maximum flow rate, if applicable)
<input type="checkbox"/> 1. Rail <input type="checkbox"/> 2. Truck <input type="checkbox"/> 3. Livestock <input type="checkbox"/> 4. Hopper: Max. Capacity: _____ <input type="checkbox"/> 5. Belt <input type="checkbox"/> 6. Over 30 lbs.: Max. Capacity: _____ <input checked="" type="checkbox"/> 7. 30 lbs. or less <input type="checkbox"/> 8. Class II (indicate on your calibration report which weight kit is Class II certified) <input type="checkbox"/> 9. Other: Please List:	<input type="checkbox"/> 1. Retail Fuel (less than 20 gal. per minute) <input type="checkbox"/> 2. High Flow Retail Fuel (20 gal. per minute or greater) <input type="checkbox"/> 3. Vehicle Tank: Max. Flow Rate: _____ <input type="checkbox"/> 4. Stationary Bulk (fuel or oil): Max. Flow Rate: _____ <input type="checkbox"/> 5. LPG <input type="checkbox"/> 6. Stationary LPG <input type="checkbox"/> 7. Fertilizer: Max. Flow Rate: _____ <input type="checkbox"/> 8. Chemical <input type="checkbox"/> 9. Anhydrous <input type="checkbox"/> 10. Loading Rack <input type="checkbox"/> 11. Other: Please List:

List below all persons employed by your company as a North Dakota Registered Service Person and the device types they are registered to certify (attach a separate sheet to list additional employees):

Permit No.	Employee	Device Types Registered to Certify (list using device type numbers from above)
<i>e.g. 1001</i>	<i>e.g. John Doe</i>	<i>e.g. Scales - 2, 3, 6, 8; e.g. Liquid - 1, 2, 6</i>
<i>1787</i>	<i>Tim Rouse</i>	<i>Scales 30lbs or less</i>

Continued on Page 2



List below all field standards (attach current calibration reports):

NIST Class F 30lbs weight set	SN 5M4R
NIST Class F 30lbs weight set	SN WS WS-KIT-3


Additional Application Items (initial where appropriate):

Standardized Test Report	<input checked="" type="checkbox"/> Copy enclosed
	<input checked="" type="checkbox"/> No change in report filed previously
Tested and Approved Sticker	<input checked="" type="checkbox"/> Copy enclosed
	<input checked="" type="checkbox"/> No change in sticker filed previously
Photocopy of Crimped Lead Wire Seal	<input type="checkbox"/> Copy enclosed
	<input checked="" type="checkbox"/> No change in crimped lead wire seal filed previously

Public Company Listing:

Include my company information on your registered service company list for public contact.  
 Yes     No

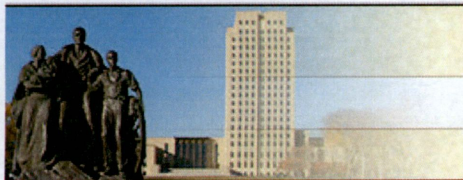
I am Penni Beall, WSM Coordinator, and have authority to represent this company. By signing this application, I declare that I have examined this form and accompanying documentation, and to the best of my knowledge and belief, the facts stated and documentation provided is true, correct, and complete.

  
 Signature

Send Completed Application and Related Documents To:

Public Service Commission  
 600 E Boulevard Ave Dept 408  
 Bismarck ND 58505-0480  
**Telephone:** (701) 328-2400  
**Fax:** (701) 328-2410

North Dakota

nd.gov Official Portal for  
North Dakota State GovernmentNorth Dakota  
LEGENDARY

# SECRETARY OF STATE NORTH DAKOTA

[Home](#) | [Business Records Search](#)

## COMPUCOM SYSTEMS, INC.

### Corporation Details

**System ID:** 7535600      **Phone:** (972) 856-3600  
**Type:** FOREIGN BUSINESS CORPORATION  
**Status:** Active & Good Standing  
**Original File Date:** 01/26/1995      **Effective Date:** 01/26/1995  
**State of Origin:** Delaware

### Nature of Business

COMPUTER SALES/SERVICE

### Principal Office

7171 FOREST LANE DALLAS, TX 75230-2306

### Registered Agent

**CORPORATION SERVICE COMPANY**  
1709 N 19TH ST STE 3  
BISMARCK, ND 58501-2121  
Established Date: Aug 09, 2010

### Generate an Annual Report To File

To Generate a Annual Report form to be filed with the Secretary of State, select the appropriate year of the report you intend to file. This report does not contain details of a report previously filed with the Secretary of State. The annual report years reflected are an indication of the various report forms available in this site and is not an indication that an entity needs to file reports for all years. Missing years indicate that the forms for the missing year have not yet been deployed to the website, or have already been removed, and can be obtained by contacting the Secretary of State.

[2016](#) (generates a forms-fillable pdf in a new pop-up window)


[Return to Search Results](#)

[Contact Us](#)[Disclaimer](#) | [Privacy Policy](#)

We use Secure Sockets Layer (SSL) encryption technology to ensure your information is secure and protected.

Will open a new window (pop-up).

W3C WAI AA, CSS, XHTML Compliant | Copyright 2006. All Rights Reserved. The State of North Dakota.



**South Dakota Department of Public Safety  
Office of Weights and Measures  
Metrology Lab**

Lab: 1500 N Garfield - E. Truck Bypass Phone: 605-773-3170  
Office: 118 West Capitol Avenue Phone: 605-773-3697  
Pierre SD 57501

## REPORT OF CALIBRATION

LAB TEST NUMBER: MP3429  
DATE OF REPORT: 03/17/2016  
DATE RECEIVED: 03/16/2016  
DATE OF TEST: 03/17/2016


**Submitted By:** CompuCom - Matt Snyder  
**Contact:** Penni Beall  
**Mailing Address:** 7171 Forest Ln.  
**City, State, Zip:** Dallas, TX 75230  
**Phone:** 855-341-1579  
**S/A Number:**


**Standards Submitted:**  
1 Rice Lake kit (7 pieces)

**Uncertainty Statement:** The combined standard uncertainty includes the standard uncertainty reported for the standard and the standard uncertainty for the measurement process. The combined standard uncertainty is multiplied by a coverage factor *k* to provide an expanded uncertainty which defines an interval having a level of confidence of approximately 95 percent. The expanded uncertainty presented in this report is consistent with the 1995 ISO/IEC Guide to the Expression of Uncertainty in Measurement. The expanded uncertainty is not to be confused with a tolerance limit for the user during application.


**Traceability statement:**  
The Standards of the SD Metrology Laboratory used for comparison are traceable to the International System of Units (SI) through the National Institute of Standards and Technology. The laboratory test number identified above is the unique report number to be used in referencing measurement traceability for artifacts identified in this report only.

This document does not represent or imply endorsement by NIST Office of Weights and Measures or any agency of the State and/or national governments. The reported test values relate only to the observations made at the time and conditions of the test. This report may not be reproduced, except in full without the written approval of this laboratory. The client must not use this document to claim product endorsement by this laboratory.

  
Ron Peterson, Metrologist

  
Date





**South Dakota Department of Public Safety**  
**Office of Weights and Measures**  
**Metrology Lab**  
 Lab: 1500 N Garfield -- E. Truck Bypass Phone: 605-773-3170  
 Office: 118 West Capitol Avenue Phone: 605-773-3697  
 Pierre SD 57501


<b>Submitted by:</b>	CompuCom - Matt Snyder	<b>Report Number:</b>	MP3429
<b>Mailing Address:</b>	7171 Forest Ln.	<b>Date Received:</b>	03/16/16
<b>City, State, Zip:</b>	Dallas, TX 75230	<b>Date tested:</b>	03/17/16
<b>Artifacts Submitted:</b>	Rice Lake Kit SN 5M4R	<b>Condition of Weights:</b>	GOOD
		<b>Temperature (c):</b>	22.5
<b>Test Method Used:</b>	SOP 8/ MODIFIED SUB, Sep 2014	<b>Humidity:</b>	46.6
<b>Equipment Used:</b>	Mettler AX205 DR/ Mettler PR503/ Valsala PTU301	<b>Pressure (mm/Hg):</b>	702.7



Treatment of artifacts prior to testing: Thermal equilibrium was obtained by placing the artifacts in the lab overnight.  
 Standards Used: SD Lab Working Standards.  
 The values reported below relate only to those observations made at the time and conditions of the test. This test report, so numbered, may not be reproduced, except in full, without approval of the laboratory. These weights were not screened for magnetism and effects of magnetism is not included in the uncertainties.  
 A weight with an "As Found" and "As Left" correction was adjusted.

Nominal	Identifier	Correction As Found	Correction As Left	Tolerance Class F	Uncertainty	k
10 lb		158 mg		450 mg	55 mg	2.06
10 lb		127 mg		450 mg	55 mg	2.06
5 lb		98 mg		230 mg	28 mg	2.05
2 lb		36 mg		91 mg	11 mg	2.06
2 lb		48 mg		91 mg	11 mg	2.06
1 lb		23.6 mg		70 mg	8.5 mg	2.05
8 oz		19.1 mg		45 mg	5.5 mg	2.05

End of Report

  
 Ron Peterson, Metrologist

03/17/2016  
Date of Report

Office of Weights and Measures  
118 W. Capitol Ave.  
Pierre, SD 57501

Phone:605-773-3697  
Fax:605-773-6631  
www.dps.sd.gov



South Dakota Department of Public Safety  
Office of Weights and Measures  
Metrology Lab  
Lab: 1500 N Garfield - E. Truck Bypass Phone: 605-773-3170  
Office: 118 West Capitol Avenue Phone: 605-773-3697  
Pierre SD 57501

## REPORT OF CALIBRATION

LAB TEST NUMBER: MP3433  
DATE OF REPORT: 03/28/2016  
DATE RECEIVED: 03/24/2016  
DATE OF TEST: 03/28/2016



**Submitted By:** CompuCom - Jeff Still  
**Contact:** Penni Beall  
**Mailing Address:** 7171 Forest Ln.  
**City, State, Zip:** Dallas, TX 75230  
**Phone:** 855-341-1579  
**S/A Number:**

**Standards Submitted:**  
1 - 11 piece avoirdupois kit

**Uncertainty Statement:** The combined standard uncertainty includes the standard uncertainty reported for the standard and the standard uncertainty for the measurement process. The combined standard uncertainty is multiplied by a coverage factor  $k$  to provide an expanded uncertainty which defines an interval having a level of confidence of approximately 95 percent. The expanded uncertainty presented in this report is consistent with the 1995 ISO/IEC Guide to the Expression of Uncertainty in Measurement. The expanded uncertainty is not to be confused with a tolerance limit for the user during application.

**Traceability statement:**  
The Standards of the SD Metrology Laboratory used for comparison are traceable to the International System of Units (SI) through the National Institute of Standards and Technology. The laboratory test number identified above is the unique report number to be used in referencing measurement traceability for artifacts identified in this report only.

This document does not represent or imply endorsement by NIST Office of Weights and Measures or any agency of the State and/or national governments. The reported test values relate only to the observations made at the time and conditions of the test. This report may not be reproduced, except in full without the written approval of this laboratory. The client must not use this document to claim product endorsement by this laboratory.


  
**Ron Peterson, Metrologist**



03/28/16  
**Date**

Office of Weights and Measures  
118 W. Capitol Ave  
Pierre, SD 57501

Phone: 605-773-3  
FAX: 605-773-6



South Dakota Department of Public Safety  
Office of Weights and Measures  
Metrology Lab

Lab: 1500 N Garfield - E. Truck Bypass Phone: 605-773-1170  
Office: 118 West Capitol Avenue Phone: 605-773-3697  
Pierre SD 57501



Submitted by: CompuCom - Jeff Still Report Number: MP3433  
Mailing Address: 7171 Forest Ln. Date Received: 03/24/16  
City, State, Zip: Dallas, TX 75230 Date tested: 03/28/16  
Artifacts Submitted: Kit W5-Kit-3 Condition of Weights: GOOD  
Temperature (c): 22.5  
Test Method Used: SOP #/ MODIFIED SUB, Sep 2014 Humidity: 46.6  
Equipment Used: Mettler AX 205 DR Mettler PR503 Weiseta PTU301 Pressure (mm/Hg): 702.7

Treatment of artifacts prior to testing: Thermal equilibrium was obtained by placing the artifacts in the lab overnight.  
Standards Used: SD Lab Working Standards.  
The values reported below relate only to those observations made at the time and conditions of the test. This test report, so numbered, may not be reproduced, except in full, without approval of the laboratory. These weights were not screened for magnetism and effects of magnetism is not included in the uncertainties.  
A weight with an "As Found" and "As Left" correction was adjusted.

Nominal	Identifier	Correction As Found	Correction As Left	Tolerance Class F	Uncertainty	<i>t</i>
5 lb	1	100 mg		230 mg	28 mg	2.06
5 lb	2	87 mg		230 mg	28 mg	2.06
5 lb	3	92 mg		230 mg	28 mg	2.06
5 lb	4	52 mg		230 mg	28 mg	2.06
5 lb	5	93 mg		230 mg	28 mg	2.06
1 lb	1	31.6 mg		70 mg	8.5 mg	2.06
1 lb	2	21.6 mg		70 mg	8.5 mg	2.06
1 lb	3	19.6 mg		70 mg	8.5 mg	2.06
1 lb	4	23.6 mg		70 mg	8.5 mg	2.06
1 lb	5	20.6 mg		70 mg	8.5 mg	2.06
8 oz		9.1 mg		45 mg	5.5 mg	2.06

  
Ron Peterson, Metrologist

03/28/2016  
Date of Report

Office of Weights and Measures  
118 W. Capitol Ave.  
Pierre, SD 57501

Phone: 605-773-3697  
Fax: 605-773-6631  
www.dps.sd.gov

United States Department of Commerce  
National Institute of Standards and Technology

Certificate of Metrological Traceability For:

# South Dakota

This laboratory has demonstrated evidence of an unbroken chain of metrological traceability of its standards to the international system of units (SI), documented measurement uncertainties, uses documented measurement procedures, successfully completed training and proficiency tests, documented calibration intervals, submitted a quality management system, and demonstrated suitable measurement assurance for the Scope listed on this certificate.

The Office of Weights and Measures Program assesses laboratories to NIST Handbook 143 - Program Handbook for State Weights and Measures Laboratories and ISO/IEC 17025:2005.

### Scope

- Mass Echelon III
  - 30 kg to 100 mg
  - 1000 lb to 0.001 lb
  - 8 oz to 0.03125 oz
- Weight Carts
- 4000 lb to 2000 lb
- Volume Transfer, II
  - 5 gal



2016

A handwritten signature in black ink, appearing to read "Carol T. Hockett".

Carol T. Hockett, Chief  
NIST Office of Weights and Measures

Effective Dates: 2016-01-01 to 2016-12-31