


Contractor: **Kennedy Scales Inc**
 11485 Xeon St NW
 Coon Rapids, MN 55448-3150

Purchase Order #: 6428-SVC
 Client: **Kennedy Scales Inc**
 Address: 11485 Xeon St NW

City & State: Coon Rapids, MN 55448
 Date Received: 07 DEC 2016
 Date Calibrated: 09 DEC 2016
 Temperature Range: 21.15 to 21.41 °C
 Pressure Range: 738.1 to 743.6 mmHg
 Relative Humidity Range: 48 to 56 %
 Air Density: 1.1581 to 1.1672 mg/cm³
 Traceable Report #: 2525077
 NIST Certificate #: 684/286541-15, 684/284451-14
 Tested By: 03, 19
 Procedure: Mass Dissemination (reference HB 952)
 Contractor Req Recall Date: 1 Year
 Primary Standard Calibration Date: 03/16/15, 11/26/13 Due: 03/15/19, 11/24/17

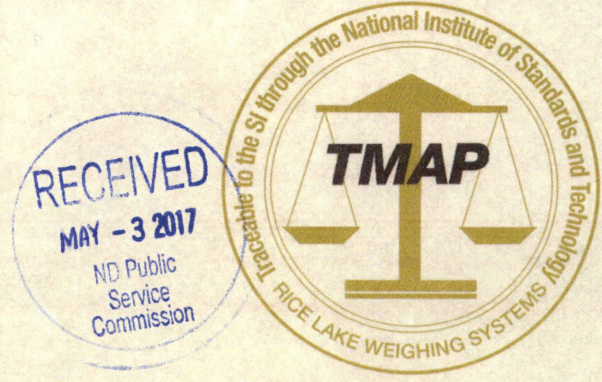

APPROVED
 PC 12-13-16

Description of Weights: 10 mg & 500 mg Leaf Weights & 1 g to 5 kg Polished Weight Set, ASTM Class 1, S/N M12

Nominal Value	Id.	Conventional Mass Corr.		Unc. ¹ K=2 (mg)	Tot. (mg)	Balance Used	Standard Set Used		Assumed Density (g/cm ³)
		As Found (mg)	As Left (mg)				Calibrated/due MM-DD-YY/MM-DD-YY	MM-DD-YY/MM-DD-YY	
10 mg		0.0023	0.0023	0.0024	0.010	503Q	L595Q	10-06-16/01-06-17	7.95
500 mg		-0.0020	-0.0020	0.0016	0.010	503Q	L595Q	10-06-16/01-06-17	7.95
1 g		0.0093	0.0093	0.0018	0.034	503Q	L595Q	10-06-16/01-06-17	7.95
2 g		0.0235	0.0235	0.0023	0.034	503Q	L595Q	10-06-16/01-06-17	7.95
2 g		0.0072	0.0072	0.0023	0.034	503Q	L595Q	10-06-16/01-06-17	7.95
5 g		0.0119	0.0119	0.0047	0.034	503Q	L595Q	10-06-16/01-06-17	7.95
10 g		0.0107	0.0107	0.0081	0.050	1470Q	L595Q	10-06-16/01-06-17	7.95
20 g		0.014	0.014	0.011	0.074	1470Q	L595Q	10-06-16/01-06-17	7.95
20 g		-0.009	-0.009	0.011	0.074	1470Q	L595Q	10-06-16/01-06-17	7.95
50 g		0.034	0.034	0.022	0.12	1470Q	L595Q	10-06-16/01-06-17	7.95
100 g		-0.070	-0.070	0.038	0.25	699Q	L595Q	10-06-16/01-06-17	7.95
200 g		0.193	0.193	0.042	0.50	699Q	L595Q	10-06-16/01-06-17	7.95
200 g		0.127	0.127	0.042	0.50	699Q	L595Q	10-06-16/01-06-17	7.95
500 g		0.386	0.386	0.071	1.2	699Q	L595Q	10-06-16/01-06-17	7.95
1 kg		0.69	0.69	0.12	2.5	699Q	L595Q	10-06-16/01-06-17	7.95
2 kg		2.15	2.15	0.45	5.0	124Q	L595Q	10-06-16/01-06-17	7.95
2 kg		1.57	1.57	0.45	5.0	124Q	L595Q	10-06-16/01-06-17	7.95
5 kg		5.23	5.23	0.80	12	124Q	L595Q	10-06-16/01-06-17	7.95
5 kg		4.95	4.95	0.80	12	124Q	L595Q	10-06-16/01-06-17	7.95

¹ Uncertainties apply to As Left values only

This report contains data not covered by the NVLAP Accreditation if the box is checked.


Check with your local state agency for certification of compliance on Legal for Trade items.
 The weight tolerance class is referenced in the Description of Weights. Unless otherwise noted, weights tested meet the requirements of the class.
 *The specifications for the weight classes can be found in NIST Handbook 105-1, ASTM E-617 or OIML R111.

Prepared By:
Rice Lake Weighing Systems
 230 West Coleman Street, Rice Lake, WI 54868
 TEL: 715-234-9171 • FAX: 715-234-6967 • www.rice-lake.com
 An ISO 9001 registered company

5 WM-16-713 Filed: 5/3/2017 Pages: 1
Calibration report - Class 1 weight kit

Dated **12 DEC 2016**

Dan Demers Metrologist



Kennedy Scales, Inc.

This document shall not be reproduced, except in full, without the GUM and include uncertainty components for reference level of confidence of approximately 95 percent.